

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

FEB 24 2011
2011-02-24
3/12/11

Supervisor/Operator Performing the Verification Procedure:

DataMaster cdm S/N 130 286 ✓

Name Det. Stan Swetzof ID# 5002 ✓ Date 2/20/11 ✓

A

Agency North pole PD Phone # 907-488-0612

Instrument Location 125 Snowman Lane, North pole, AK 99705

B


Alco S/N X124662 ✓ Target Value .087 ✓ High Pressure 550 PSI

Alco Test Values

.084 ✓
1st Alco

.084 ✓
2nd Alco

Signature

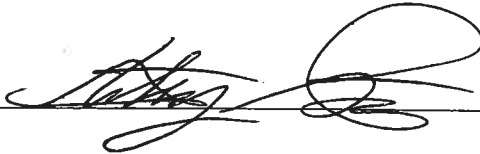


(OVER)

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

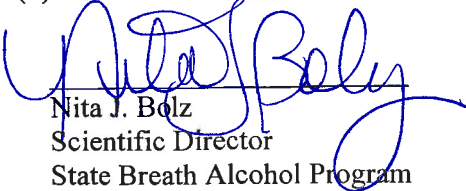

Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 18th day of MAR, 2011 Det

(Notary Seal Stamp)


Daniel L. Nicholas
Notary Public, State of Alaska
Commission Expires with Office

BT9 06/03



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130286

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130286

FEBRUARY 20, 2011

OPERATOR'S NAME:

SMETZOF-STANLEY

OPERATOR'S NUMBER: 5002

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/ID:

L

O.L. #: L

DEPT/AGENCY: NPL1

CASE/REPORT:

TEST TYPE: U

ALCO TARGET VALUE: .087

ALCO S/N: X124662

--- BREATH ANALYSIS ---

.087 ADJUSTED FOR 29.57 in
ALCO TARGET .085 23:41
BLANK TEST .000 23:42
INTERNAL STANDARD VERIFIED 23:42
ALCO TO 29.57 in .084 23:42
BLANK TEST .000 23:43
SUBJECT SAMPLE .000 23:44
BLANK TEST .000 23:45
ALCO TO 29.57 in .084 23:45
BLANK TEST .000 23:46

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130286

FEBRUARY 20, 2011

TIME 23:37

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 01/08/09

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 41c

BAROMETER: 29.57 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!@#%&'()*+,-./0123456789:;<=>?@ABCDEF
GHIJKLMNOPQRSTUVWXYZ[]^_`abdefghijklmno
pqrstuvwxyz{|}~!